


1. Preparation before using a counting chamber:

WHAT YOU NEED
Haemocytometer with cover glass
Cell suspension suitably diluted
Tally counter
Pasteur pipettes
Microscope (compound or stereo)

1. The haemocytometer is an expensive piece of equipment that must be handled carefully. To avoid getting fingerprints on the ruled areas, the counting chamber should be held by the sides and bottom only.
2. Use only the cover glass provided with the haemocytometer as a regular coverslip will NOT give accurate results.
3. Take extra care when focusing the microscope as the counting chamber is much thicker than a conventional slide. **The microscope objective, as well as the chamber and cover glass may be damaged beyond repair if the user is not careful.**
4. Clean the counting chamber gently with 70% alcohol and a lint-free wipe

Note:

The figure opposite is reprinted with the kind permission of Current Protocols in Cell Biology, John Wiley & Sons Inc. www.currentprotocols.com/protocol/cb0101

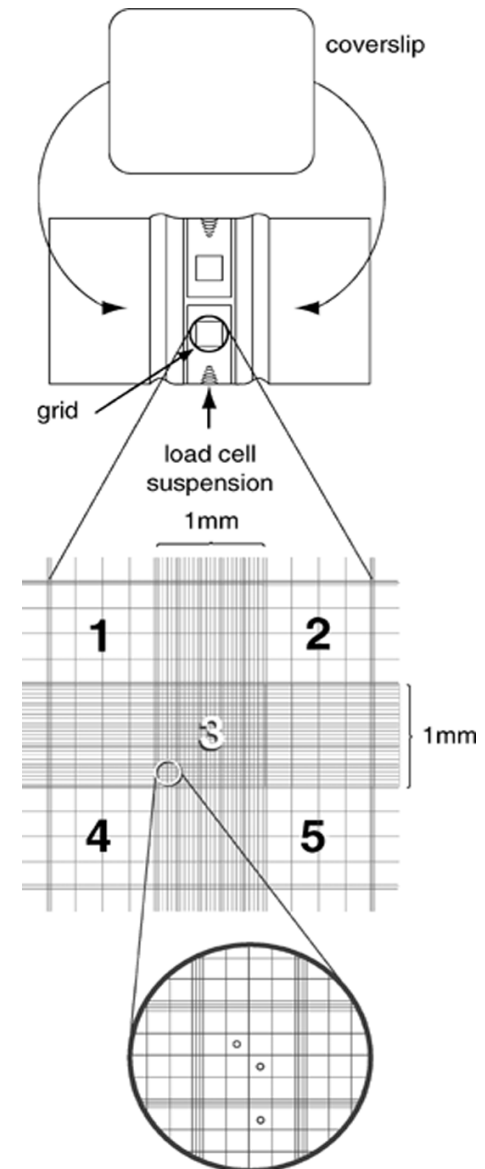

2. Protocol for using a counting chamber:

1. Moisten the shoulders of the haemocytometer and affix cover glass using gentle pressure and small circular motions. This ensures that the depth of the chamber is correct (0.1 mm).
2. Using a Pasteur pipette, place a drop of the cell suspension at the edge of the 'V' shape of the chamber. Allow the suspension to be drawn into the chamber by capillary action. ****CARE**** Do not over-fill or under-fill the chamber. Fill the opposite chamber in the same manner.
3. The rulings cover 9 mm² in a 3x3 square. The central square of the grid is ruled into 25 groups of 16 smaller squares (area of each smaller square is 0.0025 mm²) with each group separated by triple lines, the middle one of which is the boundary.

The area of the central square is: $25 \times 16 \times 0.0025 = 1 \text{ mm}^2$ and the volume is: $1 \text{ mm}^2 \times 0.1 \text{ mm} = 0.1 \text{ mm}^3$ or $0.1 \mu\text{l}$ ($1 \text{ ml} = 1000 \text{ mm}^3$).

The number of cells counted per ml = number of cells counted per square mm x dilution x 10,000.

4. To ensure accuracy of counts, a specific counting pattern must be determined. See: <http://www.ruf.rice.edu/~bioslabs/methods/microscopy/cellcounting.html>
(Reproduced with permission, a pdf 'Using a Counting Chamber' can be accessed on www.kirkhoustrust.org, click on 'Protocols'

Counting Fungal Spores: <http://www.ncbi.nlm.nih.gov/pmc/articles/PMC202674/pdf/aem00111-0126.pdf>

